

Certificate of Calibration

Nolan Recycling Ltd
 Waste Transfer Station
 The Old Quarry
 Stormy Down
 Bridgend
 CF33 4RS

Customer Ref: Weighbridge
 Location: Site
 Manufacturer: Leon
 Type: LD5218
 Serial No: L07340153
 Capacity: 50000 Kg x 20 Kg
 Next Due: April 2019

All test weights are traceable to the National Physical Standard as certified by a UKAS Accredited Laboratory

Test Weight Details

Set Number	Certificate Number
PB50-65 100-105	TR10227

Deviation / Tolerance for Compliance +/-

0 Kg - 10000 Kg	+/- 20 Kg
10000 Kg - 40000 Kg	+/- 40 Kg
40000 Kg - 50000 Kg	+/- 60 Kg

AS Found Hysteresis

Load	Loading	Deviation
0 Kg	0	0 Kg
10000 Kg	10000	0 Kg
16000 Kg	15980	-20 Kg
20000 Kg	20000	0 Kg
34240 Kg	34240	0 Kg
44240 Kg	44220	-20 Kg

Post Adjustment Hysteresis

Load	Loading	Deviation
0 Kg	0	0 Kg
10000 Kg	10000	0 Kg
16000 Kg	15980	-20 Kg
20000 Kg	20000	0 Kg
34240 Kg	34240	0 Kg
44240 Kg	44220	-20 Kg


As Found Repeatability

Zero	Load 1	Zero	Load 2	Zero	Load 3
0	6820	0	6820	0	6820

Post Adjustment Repeatability

Zero	Load 1	Zero	Load 2	Zero	Load 3
0	6820	0	6820	0	6820

Engineers Comments
 Satisfactory to tolerance.

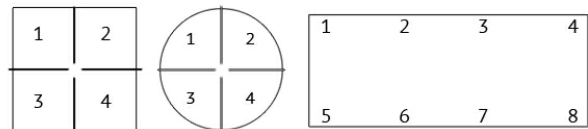

As Found Eccentric Loading

Reading	Dev	Reading	Dev
1 6820	20 Kg	2 6840	40 Kg
3 6820	20 Kg	4 6820	20 Kg
5		6	
7		8	

Post Adjustment Eccentric Loading

Reading	Dev	Reading	Dev
1 6820	20 Kg	2 6840	40 Kg
3 6820	20 Kg	4 6820	20 Kg
5		6	
7		8	

The above detailed equipment has been tested in accordance with the UKWF Guidelines and found to be within specified tolerances unless otherwise stated